


# EuroEA Elemental Analyser



AutoRun name : Zaid (6)  
 Date of Analysis : 10 Feb 2019  
 Time of Analysis : 12:19:05  
 Analysed By : EVR  
 Signed By : EVR  
 Operator Group : GRP1  
 Configuration : CHNS  
 Calibration Type : Linear

## Calibration Curve for Nitrogen

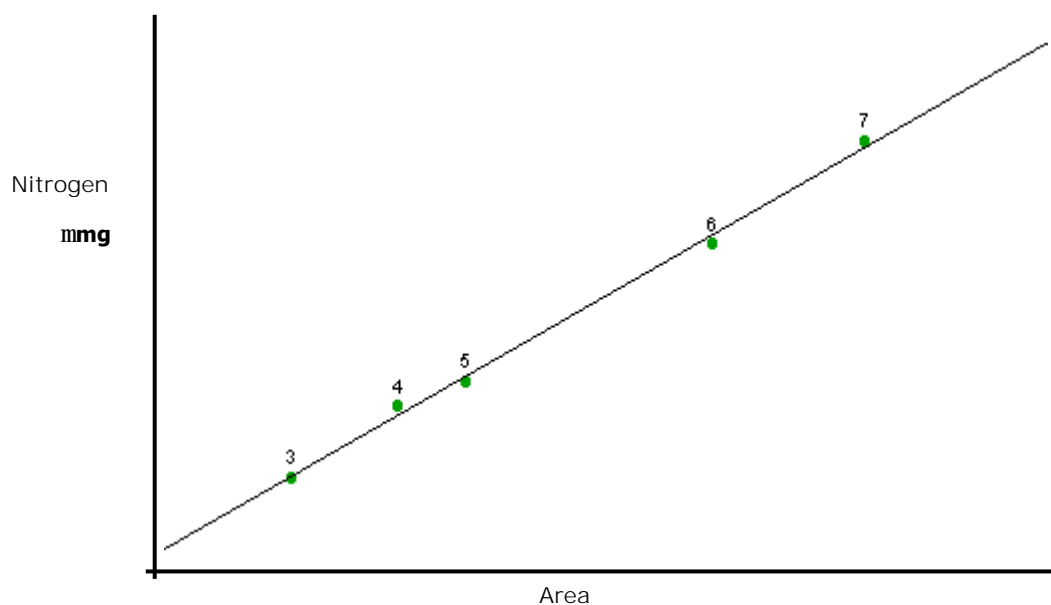

Slope	Intercept	Correlation
7.207543E-07	0.014	0.9984550

#	Name	Type	Area	N %	KFactor	Weight (mg )
3	Acetanilide	Std	67,014	10.399	-	0.603
4	Acetanilide	Std	80,362	10.172	-	0.711
5	Acetanilide	Std	88,843	10.458	-	0.750
6	Acetanilide	Std	119,940	10.516	-	0.959
7	Acetanilide	Std	139,022	10.269	-	1.116